

**Thesis**

**Workflow assessment of an augmented reality  
application for planning of perforator flaps in plastic  
reconstructive surgery: Game or game changer?**

submitted by

**Matthias Fabian Berger**

In partial fulfillment of the requirements for the degree of

**Doktor der gesamten Heilkunde  
(Dr. med. univ.)**

at the

**Medical University of Graz**

executed at the

**University department of Surgery  
Division of Plastic, Aesthetic and Reconstructive Surgery**

under the supervision of

**Assoc. Prof. Priv.-Doz. Dr. med. David Benjamin Lumenta  
Dr. med. univ. Melanie Pichlsberger**

Graz, 12.07.2023

*Declaration of Academic Integrity*

*I hereby confirm that the present diploma thesis is the result of my own independent scholarly work. I also confirm that in all cases, where material from the work of others (in books, articles, essays, dissertations, and on the internet) is acknowledged, quotations and paraphrases are clearly indicated. No material other than that cited in the reference list has been used. I have read and understood the Medical University's regulations and procedures concerning plagiarism.*

*Graz, 12.07.2023*

*Matthias Berger m.p.*

## Preface

The present thesis was written as part of my studies in Medicine at the Medical University of Graz and serves as my final project. Furthermore, I had the opportunity to publish this final project in a prestigious journal. It can be accessed at the following link: <https://journals.sagepub.com/doi/epub/10.1177/20552076231173554>.

The main objective of this study was to investigate the integration and evaluation of Augmented Reality (AR) as a technology tool in preoperative planning for the localization of perforators in autologous breast reconstruction. The present pilot study, titled VizARd, received financial support from the Austrian Research Promotion Agency (FFG) and was conducted from November 2018 to April 2021.

The term "digitalization," often referred to as the spirit of the time, describes the emergence of new processes and products by using modern information technologies. As a subfield of "Industry 4.0," digitalization is not governed by a static model but rather a dynamic trend, fueled by advancing generations of digital technologies. Augmented Reality, a subset of Extended Reality, takes digitalization to the next level, promising a digital reality. The exponential growth surrounding Extended Reality (Augmented Reality, Virtual Reality, Mixed Reality) in the capital market underscores the exponential increase in publications on the topic of Augmented Reality in medical research. The rapid growth of this industry justifies a closer examination and exploration of this predominantly abstract form of technology.

***“AR is going to take a while, because there are some really hard technology challenges there. But it will happen, it will happen in a big way, and we will wonder when it does, how we ever lived without it. Like we wonder how we lived without our phone today.”***

Tim Cook; CEO of Apple Inc.

## **Acknowledgement**

At this point, I would like to express my deep gratitude to all individuals involved who supported me during the completion of my dissertation and accompanied me throughout my six years of study.

I would like to extend my sincere thanks particularly to Assoc. Prof. Priv.-Doz. Dr. med. **David Benjamin Lumenta**, whose outstanding commitment and profound knowledge in the medical and digital field significantly contributed to the success of my work and publication. Furthermore, I would like to express my gratitude for the mutual respect and inspiring afternoons filled with great idea exchanges.

I am profoundly grateful for the immense support and motivation I received from my family during my years of study. In particular, I would like to express my sincere thanks to my parents, **Dorothea and Silvio**, as their unwavering support has greatly contributed to both my academic and personal growth.

Furthermore, I would like to thank my girlfriend **Livia**, who stood by my side with patience and resolute support throughout my years of study.

# Zusammenfassung

## **Einleitung:**

Entgegen den weltweit zunehmenden finanziellen Investitionen in Forschung und Entwicklung der Medizintechnik, offenbart sich eine unzureichende Usability und klinische Anwendbarkeit der produzierten Systeme. In dieser Studie evaluierten wir ein Augmented Reality (AR)-Setup zur präoperativen Kartierung von Perforatorgefäßen bei elektiver autologer Brustrekonstruktion.

## **Methodik:**

In diesem Pilotprojekt, das von der Österreichischen Forschungsförderungsgesellschaft (FFG) finanziert wurde, wurden Magnetresonanzangiographie (MR-A) Daten des Rumpfes verwendet, um die Scans mithilfe einer freihändig zu bedienenden Augmented-Reality-Brille auf die entsprechenden Patienten zu überlagern und somit die für die Operationsplanung relevanten Regionen zu identifizieren. Die Position des Perforators wurde anhand von MR-A-Bildgebung (MR-A-Projektion) und Doppler-Ultraschalldaten (3D-Distanz) beurteilt und in allen Fällen intraoperativ bestätigt. Die Benutzerfreundlichkeit wurde anhand der System Usability Scale (SUS) bewertet, die Datenübertragungslast wurde erfasst und die für die Softwareentwicklung aufgewendeten Arbeitsstunden wurden dokumentiert. Des Weiteren wurden die Korrelation der Bilddaten sowie die Zeitspanne von der MR-A- bis zur AR-Projektion für jeden Scan gemessen, um die Verarbeitungsdauer bis zur klinischen Einsatzbereitschaft zu ermitteln.

## **Ergebnisse:**

Alle Positionen der Perforatoren wurden intraoperativ verifiziert. Es wurde eine signifikante Korrelation (Spearman  $r = 0,894$ ) zwischen der MR-A-Projektion und den 3D-Abstandsmessungen festgestellt. Die allgemeine Benutzerfreundlichkeit (SUS) wurde mit  $67 \pm 10$  bewertet, was als mäßig bis gut eingestuft wird. Die gesamte Konfiguration für AR-Projektionen dauerte 173 Minuten, d.h. bis zur vollständigen Einsatzbereitschaft auf dem AR-Gerät pro Patient.

**Schlussfolgerung:**

In diesem Pilotprojekt kalkulierten wir Entwicklungsinvestitionen auf der Grundlage von projektbewilligten, geförderten Personalstunden mit einem mäßigen bis guten Usability-Ergebnis, das sich aus einigen Limitationen ergab: Die Bewertung basierte auf einer einmaligen Durchführung ohne vorangegangem Training, einer zeitlichen Verzögerung der AR-Visualisierungen am Körper und Schwierigkeiten bei der räumlichen AR-Orientierung. Der Einsatz von AR-Systemen bietet potenziell neue Möglichkeiten für die zukünftige chirurgische Planung. Allerdings zeigt sich das größere Potenzial von AR-Systemen im Bereich der Ausbildung, beispielsweise für Patienteninformationen oder die Schulung von Medizinstudenten und Postgraduierten. Hierbei geht es insbesondere um die räumliche Erkennung von Bilddaten in Verbindung mit anatomischen Strukturen und Operationsplanungen. Wir sind zuversichtlich, dass in Zukunft Verbesserungen in Bezug auf die Benutzerfreundlichkeit erzielt werden können. Dies kann durch detailliertere Benutzeroberflächen, schnellere AR-Hardware und auf künstlicher Intelligenz basierender Visualisierungstechniken ermöglicht werden.

## **Table of Contents**

Preface.....	1
Acknowledgement.....	2
Zusammenfassung.....	3
Table of Contents .....	5
List of Abbreviations.....	6
List of Figures .....	7
List of Tables.....	8
Introduction .....	9
Scientific work .....	10

## List of Abbreviations

3D	3 Dimensional
AR	Augmented Reality
CS	Consultant Plastic Surgeon
CT-A	Computed Tomography Angiography
DICOM	Digital Imaging and Communications in Medicine
DIEAP	Deep Inferior Epigastric Artery Perforator
FE	Finite Element
FFG	Forschungsförderungsgesellschaft
IQR	Interquartile Range
MB	Megabyte
min	Minutes
mm	Millimeters
MR-A	Magnetic Resonance Angiography
MRI	Magnetic Resonance Imaging
RGB-D	Red Green Blue-Depth
RT	Radiology Technician
SD	Standard Deviation
SE	Software Engineer
SP	Scientific Personnel
SUS	System Usability Scale
USD	US-Dollar

## List of Figures

- Figure 1 Flow chart showing patients workflow
- Figure 2 Quantitative and qualitative representation of the overall usability
- Figure 3 Transmitted data sizes in image preparation (see Table 2). Magnetic resonance imaging data (Dixon MRI DICOM T2) plus magnetic resonance angiography data (MR-A DICOM T1) data required a storage capacity of  $350 + 350 = 700$  MB. After segmentation, MRI and MR-A resulted in 1.6 MB of FE mesh images and 16 MB of masked MR-A images, respectively; 20 MB of the surface RGB-D scan images in combination with FE mesh images were saved to a 15-MB displacement field data file. Displacement field data and masked MR-A images operated as input variables for the deformation process. Deformed MR-A resulted in a final size of 4 MB ready for upload to the augmented reality (AR) system
- Figure A1 Link to YouTube video: <https://youtu.be/OelQkfsOn3c>
- Figure A2 Scatterplot between MR-A projection and 3D distance
- Figure A3 MR-A user interface
- Figure A4 MR-A layer movement by pinching two fingers
- Figure A5 Objective measurements in perforator location verification

## List of Tables

Table 1	System usability scale (SUS): Total score min = 0, max = 100
Table 2	Worksteps itemized in three categories
Table 3	Personnel-hours in software development
Table A1	Perforator measurements

## **Introduction**

This project was conducted by a team of 10 individuals from 4 distinct institutions. The subsequent section aims to delineate and reflect upon my own contribution to this project in chronological order.

### **Application for approval of the project from the Ethics Committee**

To initiate the application process with the Ethics Committee, a comprehensive project description (in accordance with the principles of Good Scientific Practice (GSP)) has been developed. Additionally, a comprehensive and explanatory annex containing all individuals and institutions involved in the project has been submitted.

### **Data collection and patient care**

Great emphasis was placed on providing intensive care to the patients voluntarily participating in the project. On the day of data collection, these patients were explicitly informed about the study procedure again. In accordance with the methodology section (Image acquisition) of this study, the patients were accompanied and instructed through the following stages:

- Preparation for MRI/MR-A (venous puncture, application of fiducials, changing clothes). Validated by a consultant plastic surgeon.
- Accompaniment and presence during the MRI/MR-A procedure.
- Identification of perforator vessels using Doppler ultrasound. Validated by a consultant plastic surgeon.
- Setup and calibration of the RGB-D camera. Validated by scientific personnel.
- Execution of the RGB-D scan. Validated by scientific personnel.

### **Patient detection and visualization of the collected data**

As depicted in the methodology and results sections of this study, data collection and preprocessing ahead, an augmented reality (AR) visualization was conducted. This encompassed the setup, calibration, and verification of the processed data using the AR headset. Validated by a consultant plastic surgeon.

### **Generating datasets and conducting a literature review**

Medical data sets comprising usability, personnel deployment, and size of transmitted data were collected, and a literature review was conducted.

### **Statistical Analysis**

Statistical analysis was conducted using SPSS (version 28; IBM Corp., Armonk, NY, USA).

### **Publication**

Writing the scientific manuscript as the primary author and submission of the paper to a reputable journal.

# Workflow assessment of an augmented reality application for planning of perforator flaps in plastic reconstructive surgery: Game or game changer?

DIGITAL HEALTH  
Volume 9: 1–11  
© The Author(s) 2023  
Article reuse guidelines:  
sagepub.com/journals-permissions  
DOI: 10.1177/20552076231173554  
journals.sagepub.com/home/dhj



Matthias Fabian Berger<sup>1,†</sup> , Raimund Winter<sup>1</sup>, Alexandru-Cristian Tuca<sup>1</sup>,  
Birgit Michelitsch<sup>1</sup>, Bernhard Schenkenfelder<sup>2</sup>, Robert Hartmann<sup>3</sup>,  
Michael Giretzlehner<sup>2</sup> , Gernot Reishofer<sup>4</sup>, Lars-Peter Kamolz<sup>1</sup>  
and David Benjamin Lumenta<sup>1,†</sup>

## Abstract

**Objective:** In contrast to the rising amount of financial investments for research and development in medical technology worldwide is the lack of usability and clinical readiness of the produced systems. We evaluated an augmented reality (AR) setup under development for preoperative perforator vessel mapping for elective autologous breast reconstruction.

**Methods:** In this grant-supported research pilot, we used magnetic resonance angiography data (MR-A) of the trunk to superimpose the scans on the corresponding patients with hands-free AR goggles to identify regions-of-interest for surgical planning. Perforator location was assessed using MR-A imaging (MR-A projection) and Doppler ultrasound data (3D distance) and confirmed intraoperatively in all cases. We evaluated usability (System Usability Scale, SUS), data transfer load and documented personnel hours for software development, correlation of image data, as well as processing duration to clinical readiness (time from MR-A to AR projections per scan).

**Results:** All perforator locations were confirmed intraoperatively, and we found a strong correlation between MR-A projection and 3D distance measurements (Spearman  $r = 0.894$ ). The overall usability (SUS) was  $67 \pm 10$  (=moderate to good). The presented setup for AR projections took 173 min to clinical readiness (=availability on AR device per patient).

**Conclusion:** In this pilot, we calculated development investments based on project-approved grant-funded personnel hours with a moderate to good usability outcome resulting from some limitations: assessment was based on one-time testing with no previous training, a time lag of AR visualizations on the body and difficulties in spatial AR orientation. The use of AR systems can provide new opportunities for future surgical planning, but has more potential for educational (e.g., patient information) or training purposes of medical under- and postgraduates (spatial recognition of imaging data associated with anatomical structures and operative planning). We expect future usability improvements with refined user interfaces, faster AR hardware and artificial intelligence-enhanced visualization techniques.

<sup>1</sup>Research Unit for Digital Surgery, Division of Plastic, Aesthetic and Reconstructive Surgery, Department of Surgery, Medical University of Graz, Graz, Austria

<sup>2</sup>RISC Software GmbH, Hagenberg, Austria

<sup>3</sup>Netural GmbH, Linz, Austria

<sup>4</sup>Radiology Lab, Department of Radiology, Medical University of Graz, Graz, Austria

<sup>†</sup>These authors contributed equally to this work.

## Corresponding author:

Raimund Winter, Research Unit for Digital Surgery, Division of Plastic, Aesthetic and Reconstructive Surgery, Department of Surgery, Medical University of Graz, Graz, Austria.

Email: r.winter@medunigraz.at



## Keywords

digital health, general, eHealth, general, electronic, general, technology, general, augmented reality, general, imaging, medicine, personalized medicine, plastic surgery

Submission date: 22 November 2022; Acceptance date: 14 April 2023

---

## Introduction

The hype for augmented reality (AR) has not only been limited to consumer technology but also found its way into the medical domain. AR – in contrast to virtual reality, where a user is immersed in a virtual world – permits an interactive and simultaneous presentation of virtual information in the real world. In a kitchen planning example, virtual reality immerses the user in a virtual environment to visualize the kitchen. By contrast, AR glasses allow to visualize virtual furniture with the user in the real kitchen observing their planned alignment.

Although AR technologies have been developed for surgical planning in different disciplines<sup>1–3</sup> and used especially in the field of neurosurgery,<sup>4</sup> their widespread application for surface markings in surgical interventions on soft tissues remains so far limited.<sup>5,6</sup> The advantages of AR for surgical planning include hands-free application, simultaneous multi-modal presentation of patient-specific data, and a focused site-centered workflow.

Healthcare and information technology have something in common, both industries are primarily centered on a target group: patients in the former or end-users in the latter. By contrast, the end-users of medical technology are predominantly clinicians, usually involved late in the development process,<sup>7</sup> where a product is closer to market readiness.<sup>8</sup> Given that predicted spending for research and development in medical technology was estimated to reach 34.3 billion USD in 2021,<sup>9</sup> the consideration of end-users only in late stages of development carries significant risks. Scientific data to support this hypothesis is difficult to find in the medical literature, since this type of data either concerns startups not making it into the market or involves access to internal entrepreneurial documents of products shelved during the end-product stage.

An important parameter for technology assessment is usability, which contains, among others, features of effectiveness, efficiency, memorability and applicability.<sup>10–13</sup> Polls by use of questionnaires have become the most popular form for usability assessments since they are less expensive than qualitative evaluations such as interviews, reproducible for follow-up purposes and provide diagnostic

information about usability issues.<sup>14–16</sup> In business models, early usability considerations have a proven benefit for reducing time spent on development<sup>17</sup> and its associated costs.<sup>18</sup>

The primary aim of this pilot study was to assess the usability of an AR project using magnetic resonance imaging and three-dimensional surface scanning on the human body during workflow and user interface development for planning of autologous abdominal-based reconstructive surgery. Secondary outcome parameters were the workload expressed in personal hours, data transfer load and time-to-clinical readiness.

## Methods

This pilot study was grant supported by the Austrian Research Society FFG (grant number: 867536 / eCall: 16967188) and approved by the institutional ethical board of the Medical University of Graz (vote #: 31-360 ex 18/19). It was conducted at the Division of Plastic, Aesthetic and Reconstructive Surgery, Department of Surgery at the Medical University of Graz between November 2018 and April 2021.

The clinical use case was the surgical planning stage of a free abdominal-tissue-based free deep inferior epigastric artery perforator flap (DIEAP flap), which is a routine procedure for autologous breast reconstruction.<sup>19</sup> Imaging modalities included magnetic resonance imaging and angiography (MRI and MR-A) for perforator visualization, three-dimensional surface scanning of the trunk for soft-tissue deformity algorithm calculation, and Doppler ultrasound exams for verification of AR-based markings. The anatomical region of interest in this study concerned the soft tissue overlaying the abdominal wall, where changes in position occur depending on the patient's posture. To calculate this deformation more accurately, an algorithm was developed, which has been published previously.<sup>20</sup> For AR visualization, we used the Magic Leap Version 1 (Magic Leap Inc., Florida, USA), which has a head-mounted display to project holograms to the headset wirelessly. Anatomical landmarks were required to manually align the deformed MRI/MR-A with the patient's trunk. The anatomic landmarks included the

---

xiphoid process, umbilicus and both anterior superior iliac spinae. The additional overlay landmarks were the oil-based fiducials (the fiducials were visible on MRI/MR-A images, on the 3D-surface scan and of course on the patients' body). The fiducials on the patient's skin were kept during the whole workflow and were used for alignment/calibration.

### Patients

Ten patients who were scheduled for elective autologous breast reconstruction using a DIEP flap were assessed for inclusion. The criteria for patient selection were as follows: patients in their first operative treatment after mastectomy; patients with a secondary operative reconstruction; and, patients must be able to provide written informed consent.

### Workflow


The pilot study workflow involved the following six steps: (1) image acquisition (MRI and MR-A, 3D-scan, Doppler ultrasound), (2) image preparation, (3) patient detection and AR visualization, (4) usability evaluation, (5) Doppler ultrasound verification of perforator location and (6) evaluation of secondary parameters (size of data transmitted and personnel costs in software development and time-to-clinical readiness) (Figure 1) [Scan the QR-Code in Figure A1 to watch a demonstration video online].

### Usability

Usability was assessed by two consultant surgeons and one resident by the System Usability Scale (SUS). The SUS is widely used and accounts for 43% of post-study questionnaires in the literature.<sup>21</sup> The 10-question paper-pencil questionnaire is based on a 5-point Likert scale (1 = strongly disagree; 5 = strongly agree). The calculated combination yields an overall usability score ranging from 0–100%.<sup>22</sup> A modified score ranking by Bangor et al. was used to interpret the overall usefulness of each patient.<sup>23</sup>

### Verification of perforator location

For objective measurements, we provided the following three lengths in Millimeters (mm) (Table A5). The 3D distance defined the distance of the ultrasound marking on the skin to its perforating vessel location on the abdominal wall. The MR-A projection defined the perpendicular distance of the MRI/MR-A, algorithm, 3D-surface scan-defined location on the skin to its perforating vessel location on the abdominal wall. The 2D distance was the distance of the two previously mentioned points on the skin. The 3D distance was defined as control.

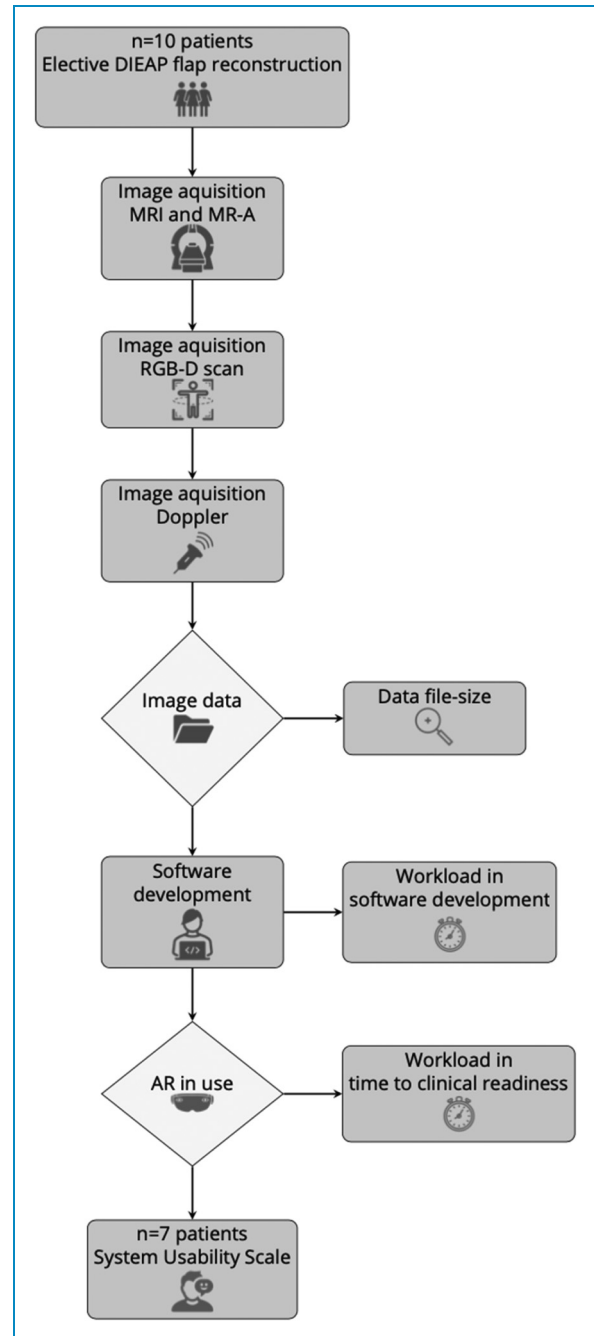

**Figure 1.** Flow chart showing patients workflow.

For objective evaluation of the obtained data, we compared the length of the MR-A projection (obtained from the MRI/MR-A data) and the 3D distance (assessed by ultrasound) (GE healthcare, Logiq E10 series, Chicago, IL, USA) in mm. The 2D distance of less than 40 mm, which described the distance between the defined perforator locations by MRI/MR-A and ultrasound, on the highly movable abdominal skin, was defined as clinically acceptable. All perforator locations were also verified intraoperatively.

### Size of data transmitted

Diagnostic imaging requires a great amount of memory in hospital IT-systems. The project challenged to decompose large DICOM file size data into small image files, AR glasses ready. DICOM is one of several medical image file formats. It is used to standardize images generated by image acquisition modalities.<sup>24</sup> To downsize DICOM to transferable file size, we used segmentation, registration and deformation processing. In every step, the image got processed, and file size data was collected. We have already published a paper that addresses the specific processing methods in detail.<sup>20</sup>

### Statistical analysis

Data was analyzed with the statistical software SPSS (version 28; IBM Corp., Armonk, NY, USA). We reported parametric data using means  $\pm$  standard deviation (SD) and non-parametric data using median (IQR, 25–75 percentiles), where appropriate. The correlation between MR-A projection and 3D distance was assessed by the Spearman coefficient.

## Results

### Patients

Following informed consent MRI and MR-A, data was obtained from 10 patients scheduled for elective autologous breast reconstruction using an abdominal-based fat and skin flap for free tissue transfer (DIEAP flap). The mean age of the finally included patients was 46.6 years (median: 49.5 years; range: 33–53 years), and the mean body mass index was 28.4 (median: 28.7; range: 19.5–35.3). All data were collected preoperatively.

### Augmented reality visualization and perforator evaluation

In the AR software app, the alignment of the processed data to the actual patient's body was performed manually for each patient. This calibration step involved the overlaying of the anatomical landmarks and fiducials before proceeding to the ultrasound verification. The user interface allowed to align and manipulate the hologram manually on top of the patient's trunk (Figure A3), as well as to manipulate the MRI's appearance by virtually changing its settings (Figure A4).

We found a strong correlation between the MR-A projection and the 3D distance measurements (Spearman  $r = 0.894$ ) (Figure A2). All but one 2D distance measurement were within the limits of the defined offset (Table A1).

### Usability

In the seven evaluated patients, the total mean score for the SUS was 67 (SD 10). Using one classification system,<sup>23</sup> the AR setup in development qualified as a 'moderate to good' system (Figure 2). The total score per question is represented in Table 1. Three patients served as participants in the proof-of-concept evaluation of the steps in the workflow, which was required by ethical board standards. The data of these three patients was not used for the usability analysis.

### Personnel deployment

Table 2 lists, in chronological order, image acquisition, image processing, patient detection and visualization, including implementation time and personnel, required for each. The total implementation time was 173 min. Five

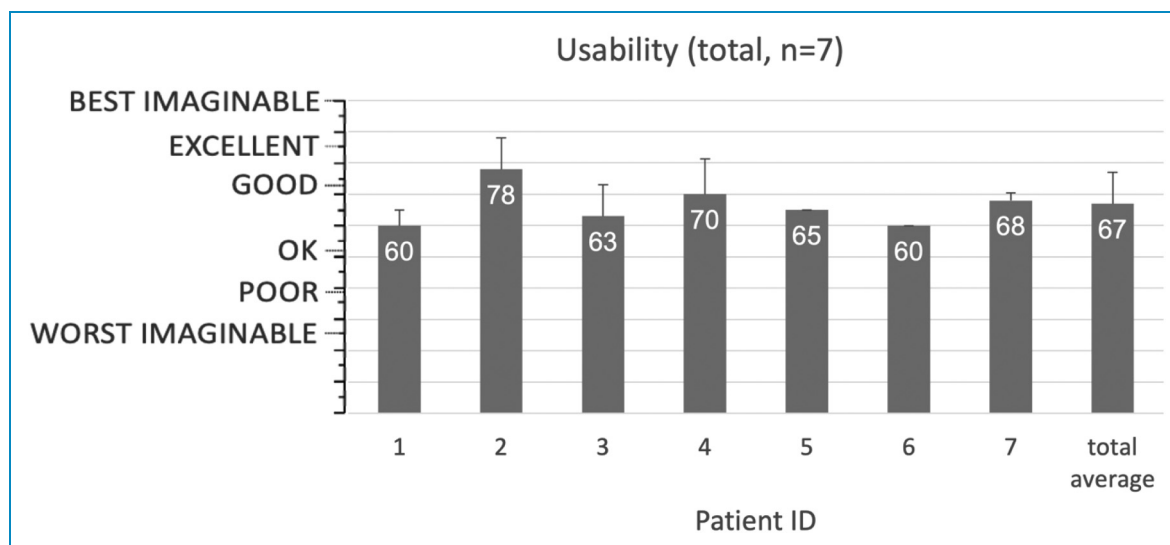


Figure 2. Quantitative and qualitative representation of the overall usability.

**Table 1.** System usability scale (SUS): Total score min = 0, max = 100.

#	SUS question	Mean (SD)
1	I think that I would like to use this system frequently.	80 (16)
2	I found the system unnecessarily complex.	37 (13)
3	I thought the system was easy to use.	75 (16)
4	I think that I would need the support of a technical person to be able to use this system.	77 (22)
5	I found the various functions in this system were well integrated.	74 (12)
6	I thought there was too much inconsistency in this system.	37 (17)
7	I would imagine that most people would learn to use this system very quickly.	68 (17)
8	I found the system very cumbersome to use.	38 (17)
9	I felt very confident using the system.	80 (14)
10	I needed to learn a lot of things before I could get going with this system.	52 (22)

modalities in the extent of 85 min in all three categorized work steps required the presence and activities of a consultant plastic surgeon (CS) (Doppler ultrasound, anonymization process, superimposition of the hologram on the patient), as well as a radiologist (preparation for MRI/MR-A, data transfer for anonymization); 45 min were required for the MR-A by two radiology technicians. The preparation of the RGB-D camera, as well as the subsequent RGB-D scan took 25 min (research assistant/scientific personnel SP). Image processing, as well as detection and visualization, required 81 min by one software engineer (Table 2). Personnel hours in software development reached a total of 2430 h, dividing 65.8% in app development and 34.2% in soft tissue calculation (Table 3).

## Discussion

The SUS of this AR-goggle-based clinical setup to superimpose MR-A data on patients for preoperative planning was rated as ‘moderate to good’ by experienced clinicians after a total of 2430 documented personnel hours for software development.


**Table 2.** Worksteps itemized in three categories.

Worksteps	Methods	t mean [min]	Personnel
Image acquisition	Preparation for MRI/MRA (venous puncture, application of fiducials, changing clothes)	15	1 CS
	MRI/MR-A	45	2 RT
	Doppler ultrasound	5	1 CS
	Setting up the RGB-D camera	10	1 SP
	RGB-D-Scan	15	1 SP
Image preparation	Transmission of data to be anonymized	2	1 CS
	Anonymization process	60	1 CS, 1 SE
	Image segmentation, -registration and -deformation	10	1 SE
Patient detection and visualization	Upload data to the AR-glasses	8	1 SE
	Superimposing the hologram on the patient	3	1 CS, 1 SE
Total		173	

CS: consultant plastic surgeon; SP: scientific personnel; RT: radiology technician; SE: software engineer.

The spatial orientation and superimposition was perceived as an asset for clinical personnel. The markings by readily applied conventional methods (e.g., Doppler probe, Doppler/duplex ultrasonography and distance from umbilicus based on CT-A/MR-A data) are sufficient to the experienced surgeon, and they considered the AR system as ‘nice, but not necessary tool for clinical practice’. Ideally, the current AR technologies can already be used for teaching purposes to improve spatial knowledge and to learn key steps during surgery for medical undergraduates or surgical residents in training either on patients or phantom models.<sup>25,26</sup> Furthermore, three-dimensional holograms in AR can be used to preoperatively enhance patient education by supporting visualizing medical content.<sup>27</sup>

Depending on a study’s purpose, there are 24 standardized usability assessment tools with different validity and

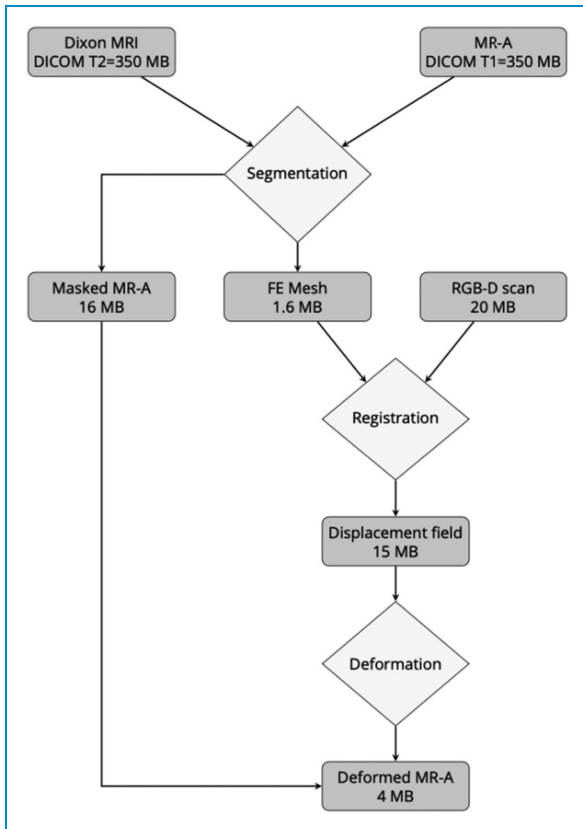

**Figure 3.** Transmitted data sizes in image preparation (see Table 2). Magnetic resonance imaging data (Dixon MRI DICOM T2) plus magnetic resonance angiography data (MR-A DICOM T1) data required a storage capacity of  $350 + 350 = 700$  MB. After segmentation, MRI and MR-A resulted in 1.6 MB of FE mesh images and 16 MB of masked MR-A images, respectively; 20 MB of the surface RGB-D scan images in combination with FE mesh images were saved to a 15-MB displacement field data file. Displacement field data and masked MR-A images operated as input variables for the deformation process. Deformed MR-A resulted in a final size of 4 MB ready for upload to the augmented reality (AR) system.

reliability schemes available.<sup>10</sup> Sauro and Lewis, both pioneering experts in the field of user experience, classified the focus of usability tools in the post-study (like the SUS) and post-task questionnaires. Alternatives suitable for our study setup were the Questionnaire for User Interaction Satisfaction,<sup>28</sup> the Software Usability Measurement Inventory<sup>29</sup> and the Post-Study System Usability Questionnaire.<sup>16,30</sup> Still additional alternatives exist,<sup>31</sup> but the SUS is nonetheless the fastest to apply during one evaluation session (less than 1–2 min), an easy-to-understand instrument for assessing a wide range of types of technology, and last but not least one of the oldest and most commonly published usability scores.<sup>32</sup>

Other authors with similar clinical endpoints examined hardware usability.<sup>33,34</sup> To our knowledge, ours is the

**Table 3.** Personnel-hours in software development.

Workload	t [h]	%
App concept/design	730	30
App programming	570	23.5
App adaption	300	12.3
Calculation of soft tissue	830	34.2
Total	2430	100

first report on AR glasses on a patient cohort while simultaneously performing a usability assessment.

The development process required significant input from clinical experts (= the potential future users), and interdisciplinary communication was key. Taking into account clinical scheduling practices, and multiple steps in a non-automated workflow from different locations, it is easy to fathom forgetting the end user along the way, causing a negative impact on user satisfaction.<sup>35</sup> Personnel hours in software development formed the greatest block of investment costs, in which one third was dedicated to the soft tissue alignment algorithm.

The amount of time invested in the concept and design process exceeded the duration for programming the AR-application by 6.5%. Therefore, the core of every project in software development depends primarily on its correct functioning, not its actual design,<sup>36</sup> which is usually oblivious to the end user.

But personnel costs for creating-, processing- and visualizing patient images were at the lower end in the project plan, and bear lessons for future endeavors.

As we traced the image preparation process, data files revealed AR upload file sizes as low as 4 MB (Figure 3). For this reason, we assume that current hardware specifications are limiting clinical use cases. In our opinion, the presented setup if automated (e.g., by linking different application programming interfaces) under a single server infrastructure and with faster AR-hardware can facilitate spatial perception for preoperative surgical markings. We believe that this will in turn positively affect future usability evaluations.

Augmented reality setups provide new modalities, notably on a visual level, which differ significantly from the status quo or state-of-the-art in the healthcare sector. To assess the potential of AR for future implementation in the operating theatre, we addressed the usability features in this pilot and kept the visual distractors in the AR environment to a minimum by providing only the necessary features for alignment and visualization in the preoperative setting. Based on the feedback and experience we made

future technical improvements notably hardware, support by artificial intelligence and especially graphical acceleration can overcome some of the usability restraints, which we observed. Overall, the presented AR setup was assessed in a pilot study and was from a usability point of view at this stage no candidate to surrogate conventional methods for the experienced surgeons. Future follow-up studies will most likely rely on improved hardware and can be assessed for better surgical planning.

## Limitations

The presented setup involved human interaction (no automation, no application programming interface used for data exchange among collaborators) in four different locations with a net workload of 173 min until clinical readiness on the AR system, and the evaluation considers therefore a pre-automation/implementation scenario.

The commonly encountered usability issues were spatial orientation for function keys in the AR system (not for the MR-A images on the patient), handling of the system functions (the system supplied manual remote was better to apply the function keys than trying within the AR environment by use of fingers), and the lagging/fluency of MRI/MR-A images.

## Conclusions

The better integrated and less complicated to use future AR systems, not only just for tech-savvy clinical youngsters but also for experienced clinicians, the higher the potential for such technology to make it into the medical device market. Understanding the current limits of the technology and its high value for educational purposes in a training context (spatial recognition and simulated execution of operations) can help developers to turn well-placed AR projects into game changer. We believe that the presented usability assessments and interdisciplinary cooperation can serve as useful guidance for future development.

**Acknowledgements:** The authors would like to thank all those who have actively collaborated in this study.


**Contributorship:** DBL, LPK, MFB and BM researched literature and conceived the study. MFB and BM were involved in protocol development, gaining ethical approval, patient recruitment and data analysis. RW, ACT, BS, RH, MG, GR and DBL were involved in patient examination and execution of study methods. MFB wrote the first draft of the manuscript. All authors reviewed and edited the manuscript and approved the final version of the manuscript.

**Declaration of conflicting interests:** The author(s) declared no potential conflicts of interest with respect to the research, authorship, and/or publication of this article.

**Ethical approval:** This study was approved by the institutional ethical board of the Medical University of Graz (vote#: 31-360 ex 18/19).

**Funding:** The author(s) disclosed receipt of the following financial support for the research, authorship, and/or publication of this article: This study was grant supported by the Austrian Research Society FFG (grant number: 867536 / eCall: 16967188).

**Guarantor:** DBL.

**ORCID iDs:** Matthias Fabian Berger  <https://orcid.org/0000-0002-1344-8408>

Michael Girtzlehner  <https://orcid.org/0000-0003-1620-1002>

## References

1. Ceccariglia F, Cerenelli L, Badiali G, et al. Application of augmented reality to maxillary resections: a three-dimensional approach to maxillofacial oncologic surgery. *J Pers Med* 2022; 12: 2047.
2. Schiavina R, Bianchi L, Chessa F, et al. Augmented reality to guide selective clamping and tumor dissection during robot-assisted partial nephrectomy: a preliminary experience. *Clin Genitourin Cancer* 2021; 19: e149–e155.
3. Posa A, Barbieri P, Mazza G, et al. Technological advancements in interventional oncology. *Diagnostics* 2023; 13: 228.
4. Costa M, Pierre C, Vivanco-Suarez J, et al. Head-Mounted augmented reality in the planning of cerebrovascular neurosurgical procedures: a single-center initial experience. *World Neurosurg* 2022; 171: e693–e706.
5. Matthews JH and Shields JS. The clinical application of augmented reality in orthopaedics: where do we stand? *Curr Rev Musculoskelet Med* 2021; 14: 316.
6. Ghaednia H, Fourman MS, Lans A, et al. Augmented and virtual reality in spine surgery, current applications and future potentials. *Spine J* 2021; 21: 1617–1625.
7. Santos IC, Gazelle GS, Rocha LA, et al. An ontology model for the medical device development process in Europe. In: *The 1st International Conference on Design and PROCesses for Medical Devices-PROMED* 2012. 2012.
8. Deutsch JR. The importance of technology design and usability. 2008.
9. Conor S. Worldwide research and development spending in medical technology from 2011 to 2024 (in billion U.S. dollars) [Internet]. Vol. 2021. 2020. <https://www.statista.com/statistics/309297/worldwide-medtech-research-and-development-spending/>.
10. Assila A and Ezzedine H. Standardized usability questionnaires: features and quality focus. *Electron J Comput Sci Inf Technol* 2016; 6: 15–31.
11. Abran A, Khelifi A, Suryan W, et al. Consolidating the ISO usability models. In: *proceedings of 11th international software quality management conference*. 2003. p. 23–5.
12. Madan A and Dubey SK. Usability evaluation methods: a literature review. *Int J Eng Sci Technol* 2012; 4: 590–599.
13. Nielsen J. *Usability engineering*. Burlington, MA: Morgan Kaufmann, 1994.

14. Sousa VE and Lopez KD. Towards usable e-health. *Appl Clin Inform* 2017; 8: 470–490.
15. Sauro J and Dumas JS. Comparison of three one-question, post-task usability questionnaires. In: proceedings of the SIGCHI conference on human factors in computing systems. 2009. p. 1599–608.
16. Sauro J and Lewis JR. *Quantifying the user experience: practical statistics for user research*. Burlington, MA: Morgan Kaufmann, 2016.
17. Donahue GM, Weinschenk S and Nowicki J. Usability is good business. *Compuware Corp Julio* 1999: 1–18.
18. Gilb T and Finzi S. *Principles of software engineering management*. Vol. 11. Reading, MA: Addison-wesley, 1988.
19. Pompei B and Farhadi J. Diep flap volume augmentation: literature review and “calzone” flap shaping technique. *J Plast Reconstr Aesthet Surg* 2020; 73: 1933–1939.
20. Schenkenfelder B, Fenz W, Thumfart S, et al. Elastic registration of abdominal MRI scans and RGB-D images to improve surgical planning of breast reconstruction. In: 2021 annual modeling and simulation conference (ANNSIM). IEEE; 2021. p. 1–12.
21. Lewis JR. The system usability scale: past, present, and future. *Int J Hum-Comput Interact* 2018; 34: 577–590.
22. Brooke J. SUS-A quick and dirty usability scale. *Usability Eval Ind* 1996; 189: 4–7.
23. Bangor A, Kortum P and Miller J. Determining what individual SUS scores mean: adding an adjective rating scale. *J Usability Stud* 2009; 4: 114–123.
24. Larobina M and Murino L. Medical image file formats. *J Digit Imaging* 2014; 27: 200–206.
25. Williams MA, McVeigh J, Handa AI, et al. Augmented reality in surgical training: a systematic review. *Postgrad Med J* 2020; 96: 537–542.
26. Molinari G, Emiliani N, Cercenelli L, et al. Assessment of a novel patient-specific 3D printed multi-material simulator for endoscopic sinus surgery. *Front Bioeng Biotechnol* 2022; 10: 974021.
27. The role and effectiveness of augmented reality in patient education: a systematic review of the literature. *Patient Educ Couns*. 2022 Jul 1; 105(7): 1917–27.
28. Chin JP, Diehl VA and Norman KL. Development of an instrument measuring user satisfaction of the human-computer interface. In: proceedings of the SIGCHI conference on Human factors in computing systems. 1988. p. 213–8.
29. Kirakowski J, Corbett M and Sumi M. The Software Usability Measurement Inventory. *Br J Educ Technol* 1993; 24: 210–212.
30. Lewis JR. Psychometric evaluation of the Post-Study System Usability Questionnaire: the PSSUQ. In: *proceedings of the human factors society annual meeting*. Los Angeles, CA: Sage Publications Sage CA, 1992, pp.1259–1260.
31. Bangor A, Kortum PT and Miller JT. An empirical evaluation of the system usability scale. *Int J Hum-Comput Interact* 2008; 24: 574–594.
32. Brooke J. SUS: a retrospective. *J Usability Stud* 2013; 8: 29–40.
33. Dennler C, Bauer DE, Scheibler AG, et al. Augmented reality in the operating room: a clinical feasibility study. *BMC Musculoskelet Disord* 2021; 22: 1–9.
34. Stifano V, Palumbo MC, Chidambaram S, et al. The use of Mixed Reality for the treatment planning of unruptured intracranial aneurysms. *J Neurosurg Sci* 2021. Epub ahead of print. DOI: 10.23736/S0390-5616.21.05356-X.
35. Mahmood MA, Burn JM, Gemoets LA, et al. Variables affecting information technology end-user satisfaction: a meta-analysis of the empirical literature. *Int J Hum-Comput Stud* 2000; 52: 751–771.
36. Hwang K. Form follows function, function follows form. *J Craniofac Surg* 2020; 31: 335.

## Appendix



**Figure A1.** Link to YouTube video: <https://youtu.be/OeIQkfs0n3c>.

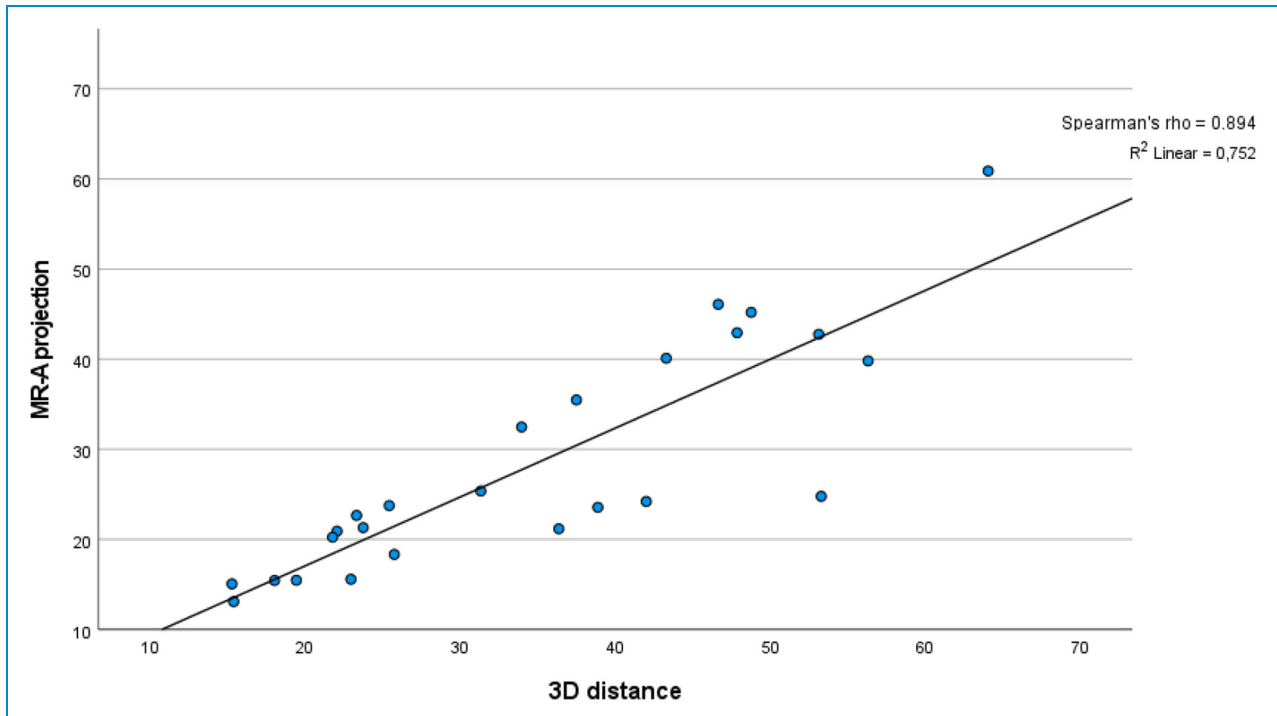


Figure A2. Scatterplot between MR-A projection and 3D distance.

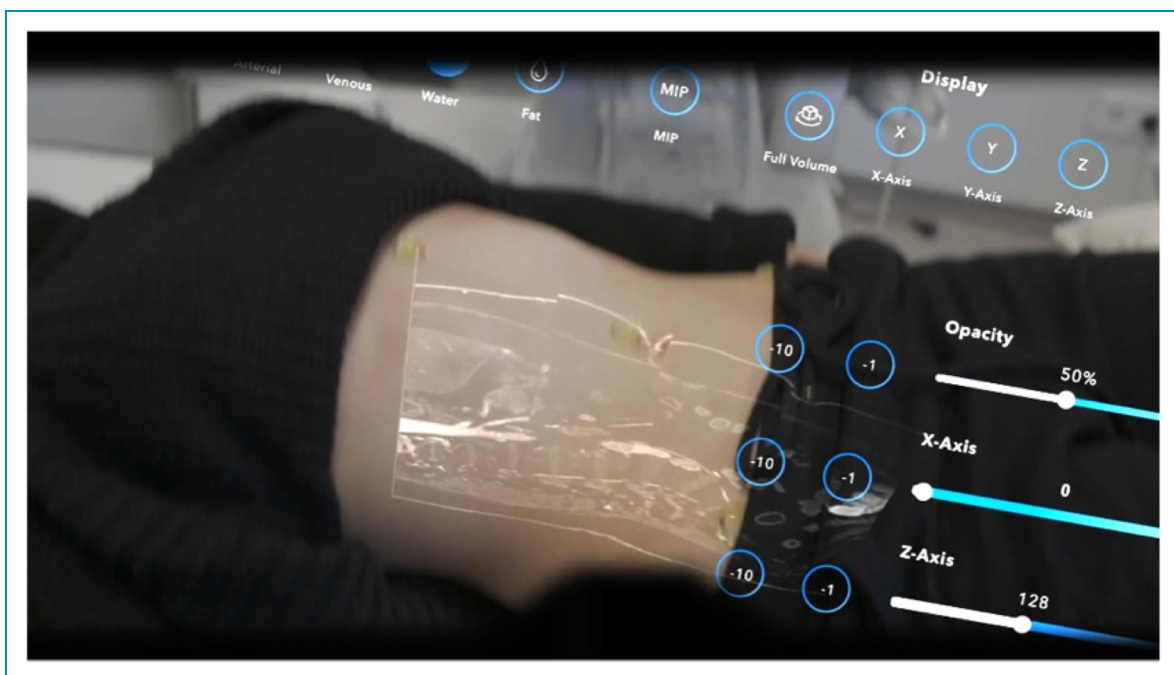


Figure A3. MR-A user interface.

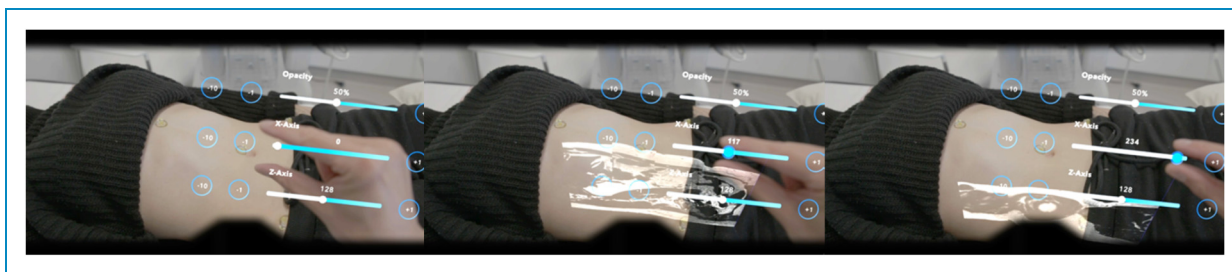


Figure A4. MR-A layer movement by pinching two fingers.

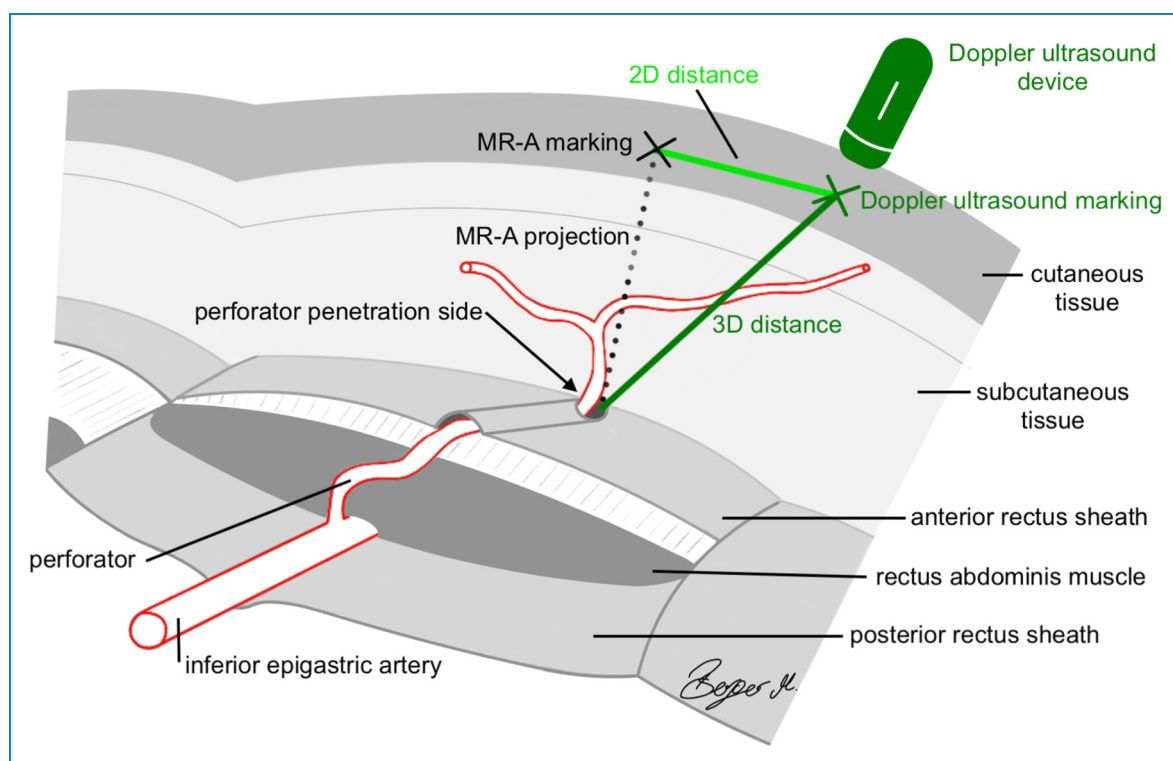


Figure A5. Objective measurements in perforator location verification.

**Table A1.** Perforator measurements.

Patient	Perforator 1			Perforator 2			Perforator 3			Perforator 4		
	MR-A projection [mm]	3D [mm]	2D [mm]	MR-A projection [mm]	3D [mm]	2D [mm]	MR-A projection [mm]	3D [mm]	2D [mm]	MR-A projection [mm]	3D [mm]	2D [mm]
P01	23.76	25.41	9.03	18.33	25.74	18.07						
P02	42.77	53.11	31.49	39.82	56.30	39.80	46.09	46.63	7.08			
P03	42.94	47.85	21.11	35.49	37.49	12.09						
P04	15.06	15.27	2.54	22.66	23.31	5.45	20.25	21.76	7.97	13.09	15.38	8.08
P05	20.92	22.05	6.98	32.48	33.95	9.89	24.78	53.28	47.16			
P06	21.18	36.35	29.54	25.37	31.32	18.36						
P07	15.57	22.94	16.85	21.31	23.74	10.45						
P08	60.89	64.05	19.84									
P09	24.21	41.99	34.31	15.46	19.42	11.76	15.44	18.02	9.29			
P10	23.56	38.87	30.91	40.11	43.28	16.26	45.21	48.76	18.26			